395 396
607/90
PATENT OFFICE
JAN 24 1939

INSTRUCTIONS
FOR INSTALLING
STERILAMP* FIXTURES

To simplify the installation problem of Westinghouse STERILAMPS, two standard types of fixtures have been designed.

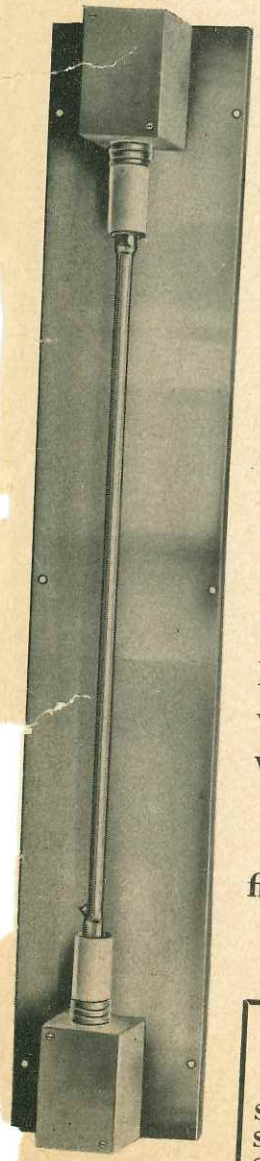

TYPE NOS. SB-10, SB-20, SB-30

This type of fixture is designed for wall or ceiling mounting where it is advisable to direct the radiation from the STERILAMP. It consists of a highly efficient flat Alzac Aluminum Reflector. This reflector utilizes radiations which would normally be absorbed by ceiling or walls. The terminal boxes are provided with convenient Knockouts for easy wiring.

All exposed metal is specially finished to withstand corrosion.

OVERALL SIZES	Length	Width	Height	Use With Sterilamps Nos.
SB-10	24″	6″	2¼″	WL 782-10
SB-20	34″	6″	2¼″	WL 782-20
SB-30	44″	6″	2¼″	WL 782-30

TYPE NOS. SC-10, SC-20, SC-30

This type of fixture is designed for use in refrigerated display cases of all types. It is attractively finished and will withstand corrosion. The open design permits the lamp to be seen by customers, thus having a distinct merchandising appeal. The two tie rods serve as a protection to the lamp.

Convenient Knockouts are provided in the terminal boxes and suitable hardware is provided for mounting in wood, metal or glass cases.

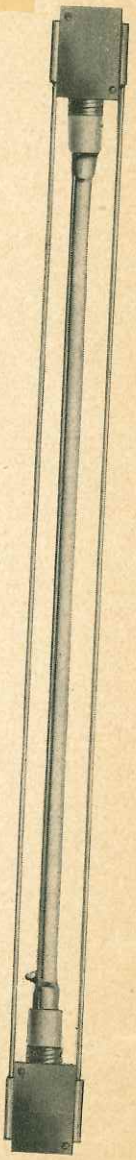

OVERALL SIZES	Length	Width	Height	Use With Sterilamps Nos.
SC-10	24″	2⅝″	2¼″	WL 782-10
SC-20	34″	2⅝″	2¼″	WL 782-20
SC-30	44″	2⅝″	2¼″	WL 782-30

lemark Reg. U. S. Pat. Off.

607/90

WIRING INSTRUCTIONS

All wiring from Power Unit to fixtures should be in metal conduit with one conductor per conduit. Conductor should not be less than No. 14 wire with 5,000 volt insulation. Connections to the sockets are easily made by removing the cover plate on the terminal boxes.

Cover plate screws are easily removed. To remove socket from holder unscrew metal ferrule. This permits socket to be removed from inside of box. Unscrew and remove back cap on socket. Connection is made to screw terminal in base of socket after sliding cap over connecting wire. Replace cap and insert socket in mounting hole in box. Lamp may then be inserted in sockets and metal ferrules tightened to rigidly position sockets in boxes. Replace cover plates. All wiring should conform to Article 600 of National Electrical Code.

For prices and further information write to

WESTINGHOUSE LAMP DIVISION

WESTINGHOUSE

ELECTRIC & MANUFACTURING COMPANY

SPECIAL PRODUCTS SALES DEPARTMENT

BLOOMFIELD, NEW JERSEY

or the following

DISTRICT OFFICES

426 Marietta Street ..... ATLANTA, GA.
20 No. Wacker Drive ..... CHICAGO, ILL.
411 No. 7th Street ..... ST. LOUIS, MO.
150 Broadway ..... NEW YORK, N. Y.
306 Fourth Avenue ..... PITTSBURGH, PENNA.
1 Montgomery Street ..... SAN FRANCISCO, CAL.

M-624-5M
MARCH 15, 1938

607/90

INSTRUCTIONS
FOR INSTALLING
STERILAMP* FIXTURES

To simplify the installation problem of Westinghouse STERILAMPS, two standard types of fixtures have been designed.

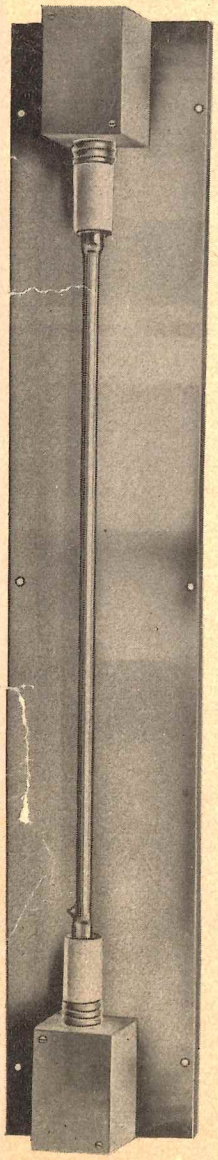

TYPE NOS. SB-10, SB-20, SB-30

This type of fixture is designed for wall or ceiling mounting where it is advisable to direct the radiation from the STERILAMP. It consists of a highly efficient flat Alzac Aluminum Reflector. This reflector utilizes radiations which would normally be absorbed by ceiling or walls. The terminal boxes are provided with convenient Knockouts for easy wiring.

All exposed metal is specially finished to withstand corrosion.

OVERALL SIZES	Length	Width	Height	Use With Sterilamps Nos.
SB-10	24″	6″	2¼″	WL 782-10
SB-20	34″	6″	2¼″	WL 782-20
SB-30	44″	6″	2¼″	WL 782-30

TYPE NOS. SC-10, SC-20, SC-30

This type of fixture is designed for use in refrigerated display cases of all types. It is attractively finished and will withstand corrosion. The open design permits the lamp to be seen by customers, thus having a distinct merchandising appeal. The two tie rods serve as a protection to the lamp.

Convenient Knockouts are provided in the terminal boxes and suitable hardware is provided for mounting in wood, metal or glass cases.



OVERALL SIZES	Length	Width	Height	Use With Sterilamps Nos.
SC-10	24″	2⅝″	2¼″	WL 782-10
SC-20	34″	2⅝″	2¼″	WL 782-20
SC-30	44″	2⅝″	2¼″	WL 782-30

607/90

ark Reg. U. S. Pat. Off.

WIRING INSTRUCTIONS

All wiring from Power Unit to fixtures should be in metal conduit with one conductor per conduit. Conductor should not be less than No. 14 wire with 5,000 volt insulation. Connections to the sockets are easily made by removing the cover plate on the terminal boxes.

Cover plate screws are easily removed. To remove socket from holder unscrew metal ferrule. This permits socket to be removed from inside of box. Unscrew and remove back cap on socket. Connection is made to screw terminal in base of socket after sliding cap over connecting wire. Replace cap and insert socket in mounting hole in box. Lamp may then be inserted in sockets and metal ferrules tightened to rigidly position sockets in boxes. Replace cover plates. All wiring should conform to Article 600 of National Electrical Code.

For prices and further information write to

WESTINGHOUSE LAMP DIVISION

WESTINGHOUSE

ELECTRIC & MANUFACTURING COMPANY

SPECIAL PRODUCTS SALES DEPARTMENT

BLOOMFIELD, NEW JERSEY

or the following

DISTRICT OFFICES

426 Marietta Street ..... ATLANTA, GA.
20 No. Wacker Drive ..... CHICAGO, ILL.
411 No. 7th Street ..... ST. LOUIS, MO.
150 Broadway ..... NEW YORK, N. Y.
306 Fourth Avenue ..... PITTSBURGH, PENN
1 Montgomery Street ..... SAN FRANCISCO, CAL.